

(19) World Intellectual Property
Organization
International Bureau



(43) International Publication Date
11 March 2004 (11.03.2004)

PCT

(10) International Publication Number
WO 2004/019782 A1

(51) International Patent Classification⁷: A61B 6/03,
G06T 17/00

(21) International Application Number:
PCT/FI2003/000625

(22) International Filing Date: 27 August 2003 (27.08.2003)

(25) Filing Language: English

(26) Publication Language: English

(30) Priority Data:
20021532 28 August 2002 (28.08.2002) FI

(71) Applicant (for all designated States except US): INSTRUMENTARIUM CORPORATION [FI/FI]; Nahkelantie 160, FIN-04301 Tuusula (FI).

(72) Inventors; and

(75) Inventors/Applicants (for US only): SILTANEN, Samuli


[FI/FI]; Yrjökatu 38 B 22, FIN-00100 Helsinki (FI). SOMERSALO, Erkki [FI/FI]; Nordeskiöldinkatu 9 A 27, FIN-00250 Helsinki (FI). KOLEHMAINEN, Ville [FI/FI]; Maljalahdenkatu 14 C 21, FIN-70100 Kuopio (FI). LASSAS, Matti [FI/FI]; Maasälväntie 8 A 43, FIN-00710 Helsinki (FI). KAIPIO, Jari [FI/FI]; Sandelsinkatu 29, FIN-70500 Kuopio (FI).

(74) Agent: LEITZINGER OY; Tammasaarenkatu 1, FIN-00180 Helsinki (FI).

(81) Designated States (national): AE, AG, AL, AM, AT (utility model), AT, AU, AZ, BA, BB, BG, BR, BY, BZ, CA, CH, CN, CO, CR, CU, CZ (utility model), CZ, DE (utility model), DE, DK (utility model), DK, DM, DZ, EC, EE (utility model), EE, ES, FI (utility model), FI, GB, GD, GE, GH, GM, HR, HU, ID, IL, IN, IS, JP, KE, KG, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, MA, MD, MG, MK, MN, MW, MX, MZ, NI, NO, NZ, OM, PG, PH, PL, PT (utility model), PT, RO, RU, SC, SD, SE, SG, SK (utility model),

[Continued on next page]

(54) Title: METHOD AND ARRANGEMENT FOR MEDICAL X-RAY IMAGING AND RECONSTRUCTION FROM SPARSE DATA

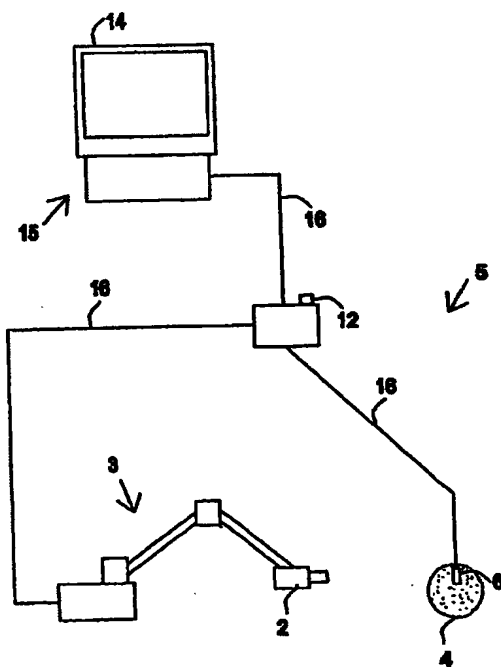

$$p(x|m) = \frac{p_{pr}(x)p(m|x)}{p(m)} \quad (I)$$

(57) Abstract: The invention relates to a medical X-ray device 5 arrangement for producing three-dimensional information of an object 4 in a medical X-ray imaging medical X-ray device arrangement comprising an X-ray source 2 for X-radiating the object from different directions and a detector 6 for detecting the X-radiation to form projection data of the object 4. The medical X-ray device 5 arrangement comprises:-means 15 for modelling the object 4 mathematically independently of X-ray imaging -and means 15 for utilizing said projection data and said mathematical modelling of the object in Bayesian inversion based on Bayes' formula (I) to produce three-dimensional information of the object, the prior distribution ppr(x) representing mathematical modelling of the object, the object image vector x, which comprise values of the X-ray attenuation coefficient inside the object, m representing projection data, the likelihood distribution p(mlx) representing the X-radiation attenuation model between the object image vector x and projection data m, p(m) being a normalization constant and the posteriori distribution p(x|m) representing the three-dimensional information of the object 4.



SK, SL, SY, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ,
VC, VN, YU, ZA, ZM, ZW.

SE, SI, SK, TR), OAPI patent (BF, BJ, CF, CG, CI, CM,
GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).

(84) **Designated States (regional):** ARIPO patent (GH, GM,
KE, LS, MW, MZ, SD, SL, SZ, TZ, UG, ZM, ZW),
Eurasian patent (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM),
European patent (AT, BE, BG, CH, CY, CZ, DE, DK, EE,
ES, FI, FR, GB, GR, HU, IE, IT, LU, MC, NL, PT, RO,

Published:

— with international search report

*For two-letter codes and other abbreviations, refer to the "Guid-
ance Notes on Codes and Abbreviations" appearing at the begin-
ning of each regular issue of the PCT Gazette.*

Method and arrangement for medical X-ray imaging

BACKGROUND OF THE INVENTION

5 Three-dimensional X-ray imaging is based on taking several 1-D or 2-D projection images of a 3-D body from different directions. If 1-D projection images are available from all around a 2-D slice of the body with dense angular sampling, the inner structure of the slice can be determined. This is known as Computerized Tomography (CT) imaging technology, which is
10 widely used in medicine today. A crucial part of CT technology is the reconstruction algorithm taking the X-ray images as argument and producing a voxel representation of the 3-D body.

In many practical cases X-ray projection images are available only from a
15 limited angle of view. A collection of X-ray images of a 3-D body is called sparse projection data if (a) the images are taken from a limited angle of view or (b) there are only a small number of images. Sparse projection data does not contain sufficient information to completely describe the 3-D body.

20 However, some a priori information about the body is typically available without X-ray imaging. Combining this information with sparse projection data enables more reliable 3-D reconstruction than is possible by using only the projection data.

25 Traditional reconstruction algorithms such as filtered backprojection (FBP), Fourier reconstruction (FR) or algebraic reconstruction technique (ART) do not give satisfactory reconstructions from sparse projection data. Reasons for this include requirement for dense full-angle sampling of data, difficulty to use a priori information for example nonnegativity of the X-ray attenuation
30 coefficient and poor robustness against measurement noise. For example the FBP method relies on summing up noise elements with fine sampling, leading to unnecessarily high radiation dose.

BRIEF DESCRIPTION OF THE INVENTION

The aim of the invention is to overcome the problems met in 3-D reconstruction of the body that occur when using traditional reconstruction algorithms with sparse projection data. This is achieved by a method for producing three-dimensional information of an object in medical X-ray imaging in which method the object is modelled mathematically independently of X-ray imaging. The object is X-radiated from at least two different directions and the said X-radiation is detected to form projection data of the object. Said projection data and said mathematical modelling of the object are utilized in Bayesian Inversion based on Bayes' formula

$$p(x | m) = \frac{p_{pr}(x)p(m | x)}{p(m)}$$

to produce three-dimensional information of the object, the prior distribution $p_{pr}(x)$ representing mathematical modelling of the object, x representing the object image vector, which comprises values of the X-ray attenuation coefficient inside the object, m representing projection data, the likelihood distribution $p(m|x)$ representing the X-radiation attenuation model between the object image vector x and projection data m , $p(m)$ being a normalization constant and the posteriori distribution $p(x|m)$ representing the three-dimensional information of the object.

The invention also relates to a medical X-ray device arrangement for producing three-dimensional information of an object in a medical X-ray imaging, said medical X-ray device arrangement comprises:

- means for modelling the object mathematically independently of X-ray imaging
- an X-ray source for X-radiating the object from at least two different directions,
- a detector for detecting the X-radiation to form projection data of the object,

- and means for utilizing said projection data and said mathematical modelling of the object in Bayesian inversion based on Bayes' formula

$$p(x | m) = \frac{p_{pr}(x)p(m | x)}{p(m)}$$

to produce three-dimensional information of the object, the prior distribution
5 $p_{pr}(x)$ representing mathematical modelling of the object, x representing the
object image vector, which comprises values of the X-ray attenuation
coefficient inside the object, m representing projection data, the likelihood
distribution $p(m|x)$ representing the X-radiation attenuation model between
the object image vector x and projection data m , $p(m)$ being a normalization
10 constant and the posteriori distribution $p(x|m)$ representing the three-
dimensional information of the object.

The invention is based on that biological tissues have that kind of statistical a
priori information that this information can be utilized successfully with
15 bayesian inversion in medical x-ray imaging. The suitable a priori information
makes possible to model the biological tissue mathematically accurately
enough and independently of X-ray imaging. From biological tissue it is
possible to compile qualitative structural information which makes it possible
to utilize the bayesian method successfully to solve the problems in medical
20 three-dimensional x-ray imaging. There are certain regularity in biological
tissues and this regularity is useful especially with the bayesian method.

For example 10 x-ray images is taken from breasts of different persons.
From these x-ray images is noticed that there is much similarity in the
25 statistical structure of the breasts between different people. In other words
biological tissues and x-ray images taken from the biological tissues has
similar or almost similar statistical structure between different persons.

With Bayesian inversion it is possible to utilize a priori information efficiently
30 in 3-D reconstruction from sparse projection data, because the suitable a
priori information from the biological tissue makes possible to model the

biological tissue mathematically accurately enough and independently of X-ray imaging. Any collection of projection data can be used in the reconstruction. Application-dependent a priori knowledge can be used to regularize the ill-posed reconstruction problem.

5

This invention improves the quality of 3-D reconstructions over traditional methods. In addition, the number of radiographs can be minimized without compromising quality of the reconstruction. This is very important in medical applications since the X-ray dose of the patient can be lowered.

10

BRIEF DESCRIPTION OF THE FIGURES

Figure 1 shows a simple example of X-ray imaging.

15 Figures 2A -2B show a difference between global tomography and local tomography.

Figures 3A – 3B show different types of sparse projection data. Every black dot represents a location of the X-ray source for taking one projection image.

20

Figures 4A - 4B show examples of parts of boundaries and cracks of an object visible and invisible without a priori information.

25 Figure 5 illustrates "pencil beam" X-ray attenuation model.

Figure 6 is basic flow chart of the method according to the invention.

Figure 7 is an intraoral X-ray device arrangement presenting one preferred embodiment of the invention.

30

Figure 8 shows a measurement geometry of dental limited-angle tomography with a digital Intraoral sensor.

5 Figure 9 shows results of 3D reconstruction of head phantom in the first preferred embodiment.

DETAILED DESCRIPTION OF THE INVENTION

10 In practical imaging situations X-ray images are not always available from all around the body. The body might be visible only from certain directions due to imaging geometry. For example this is the case in 3-D mammography with the breast compressed against the detector, or in Intraoral dental imaging with the detector inside the patient's mouth. This situation is called limited-angle tomography. Also, the region of interest might be surrounded by tissue
15 that need not be imaged, like in extraoral dental imaging. This situation is called local tomography. In addition the number of radiographs should be minimized in medical applications for reducing the X-ray dose of the patient.

20 In the preferred embodiments of the invention Bayesian Inversion algorithms are used to create a new type of 3-D medical X-ray imaging. It is intermediate between a projection radiograph and a full computed tomography scan. Two steps are needed to perform successfully such imaging: In step one, the doctor (a) collects all the prior information he or she has on the tissue of interest, and (b) takes the minimum number of
25 radiographs containing the desired 3D information. In step two, a tomographic algorithm based on Bayesian Inversion is used for 3D reconstruction. The algorithm contains two separate mathematical models. First, all a priori information (i.e. information that is independent of X-ray imaging) is used to model the unknown object mathematically. The model is
30 put into the form of prior distribution in Bayes' formula. Second, the measurement is modelled mathematically. This involves the geometry of the imaging device, position of the detector and X-ray source during the

exposure of each projection image and a model for X-ray attenuation inside tissue. The mathematical model of the measurement is put into the form of likelihood distribution in Bayes' formula.

5 In figure 1 is shown a simple example of X-ray imaging, where an X-ray source 2 is placed on one side of an object 4 under imaging. Radiation passes through the object and is detected by a detector 6 on the other side. The X-ray source is for example a X-ray source of an intraoral X-ray source of a dentist, of a dental panoramic X-ray device, of a surgical C-arm X-ray
10 device, of a mammography device or of any other medical X-ray device and the detector 6 is a detector of some of those devices. Usually the detector 6 is a digital sensor that can be thought of as a 2-D array of almost pointlike detectors.

15 The 3-D body under imaging is modelled by nonnegative X-ray attenuation coefficient. The value gives the relative intensity loss of the X-ray travelling within a small distance dr :

$$\frac{dI}{I} = -x(r)dr$$

(1)

20 The X-radiation has initial intensity I_0 when entering the object 4 and a smaller intensity I_1 when exiting the object. The following equation shows the attenuation law:

$$\int_L x(r)dr = - \int_L \frac{I'(r)}{I(r)} dr = \log I_0 - \log I_1$$

25

(2)

where initial intensity I_0 is known by calibration, and intensity after object I_1 is known from the corresponding point value in a projection image. Thus the measured data is the integral of x along the line L .

- 5 In the above model it is not taken into account (a) scattering phenomena resulting in X-rays changing their direction, or (b) the dependency of attenuation on the X-ray spectrum resulting in low-energy photons being more easily attenuated than high-energy ones. Effect (b) causes errors in measurements and is sometimes referred to as beam hardening. More
10 detailed models can be utilized in Bayesian inversion to overcome (a) and (b).

In medical imaging the geometrical arrangements of the X-ray source and digital sensor vary according to the diagnostic task and equipment. Figures
15 2A-2B and 3 illustrate the types of tomographic data resulting from different imaging situations. For clarity, here are presented two-dimensional examples; similar situations can be considered in 3-D.

In figure 2A-2B are shown two cases according to whether the whole object
20 4 is fully visible in each projection or not. These cases are called global tomography and local tomography, respectively. In figure 2B is radiated only ROI (Region Of Interest) 8.

The types of data described in figures 3A – 3B cover a large range of specific
25 imaging tasks. The choice of data collection dictates what kind of features and details it is easiest to reconstruct reliably from the data. Thus the choice of projection views must be made according to the diagnostic task at hand. In traditional CT imaging, projections are taken from all around the object 4. In the preferred embodiments of the invention radiation dose is lowered by
30 sampling the angular variable more sparsely. Figure 3A presents more dense angular data with full angle and limited angle measurements. Figure 3B

presents more sparse angular data, also with full and limited angles of measurement.

5 In figures 4A and 4B there are presented examples of parts of boundary and cracks that are visible or undetectable in reconstruction without a priori information. Figure 4A there is an object 4 under imaging with edge on the surface of the object. The edge is detectable on the leftmost position where the edge is more parallel to the direction of the X-rays. In the figure 4B there is a crack inside of the object 4. The crack is detectable in the leftmost
10 position parallel to the angle of measurement.

The main idea in Bayesian inversion method is to consider the inverse problem as a problem of statistical inference. All variables are redefined to be random variables. The randomness reflects uncertainty of their actual values
15 and the degree of uncertainty is coded in the probability distributions of these random variables.

When modelling the measurement mathematically the X-ray attenuation model and the observation can be assumed linear. The model is presented in
20 the following equation.

$$(3) \quad m = Ax + e,$$

where the variables m , x and e are random variables.

The matrix A comes from the pencil beam model for the X-ray attenuation.
25 This is presented in figure 5. There the unknown 3-D body of the object 4 is divided into small voxels 10, and the matrix A contains the lengths of the path of the X-ray inside each voxel. In this way the integral in formula (2) is approximated with a simple numerical quadrature.

30 Assume now that the object image vector x and the noise are jointly independent random variables. The conditional probability distribution of x given the measurement m is given by Bayes' formula in the form

$$p(x | m) = \frac{p_{pr}(x) p_{noise}(m - Ax)}{p(m)},$$

(4)

where $p(m)$ is a normalization constant. The density $p(x|m)$ is called the posteriori distribution of x . $p_{noise}(m-Ax) = p(m|x)$ is a likelihood distribution representing the X-radiation attenuation model between the object image
 5 vector x and projection data m .

The density p_{pr} , called the prior distribution of x , is designed to contain all possible information available of the actual object 4 independently of X-ray imaging. It is crucial, in contrast to several classical regularization methods,
 10 that the choice of the prior distribution should not be based on the projection data. The rule of thumb in the design of prior distributions is that typical image vectors (say, of some existing library) should have high prior probability while atypical or impossible ones should have low or negligible probability.

15

In the framework of the Bayesian inversion theory, the posterior distribution in formula (4) represents the complete solution of the 3D reconstruction problem.

20 To produce an image of the object 4 based on the posterior distribution, several alternatives exist. The most common ones are the maximum a posteriori estimator (MAP) and conditional mean estimator (CM). They are defined by the formulas

$$25 \quad p(x_{MAP} | m) = \max p(x | m),$$

(5)

where the maximum on the right hand side is taken over all x , and

$$x_{\text{CM}} = \int xp(x | m)dx.$$

5 (6)

Finding the MAP estimator is an optimization problem while finding the CM estimator is a problem of integration.

10 In figure 6 is presented a basic flow chart of the method according to the invention. In method step 600 the object is modelled mathematically independently of X-ray imaging. In method step 602 the object is X-radiated from at least two different directions. In method step 604 the said X-radiation is detected to form projection data of the object. In method step 606 said projection data and said mathematical modelling of the object are
15 utilized in Bayesian inversion based on Bayes formula to produce three-dimensional information of the object. The method step 600 is also possible to perform after method step 602 or 604.

20 In the first preferred embodiment of the invention is presented an application to dental radiology.

X-ray projection images are conventionally used in dental radiology. However, certain diagnostic tasks require more precise knowledge of the 3D structure of tissue than is available in two-dimensional radiographs. Such
25 tasks include implant planning and detection of bone loss between tooth roots.

In figure 7 is presented an intraoral X-ray device 5 arrangement presenting the first preferred embodiment of the invention. It is important to notice that
30 this is only an example of the medical X-ray device 5 arrangement where the invention is possible to be utilized.

The medical x-ray device 5 in the preferred embodiments of the invention is for example a dental panoramic X-ray device, a surgical C-arm X-ray device or a mammography device.

- 5 In the first preferred embodiment of the invention the articulated arm arrangement 3 moves the X-ray source 2 to the right position. The X-radiation begins by pressing the exposure button 12. The X-ray source 2 X-radiates the object 4, which is for example teeth of a patient. The detector 6 detects the X-radiation. The image information which is got by detecting the
- 10 X-radiation is sent by communication link 16 to the computer 14. The computer comprises the software means 15 to process the image information according to the invention. There can be more than one computer 14 and also the software means 15 can situate in more than one computer 14. For example the first computer 14 is computer which is used in x-ray imaging.
- 15 The second computer 14 is computer which is used in processing the image information according to the invention. It is possible to have the second computer 14 far away from the actual medical x-ray device 5. For simplicity in figure 7 is shown only one computer 14.
- 20 In the first preferred embodiment (Fig. 7) of the invention, the dentist's X-ray equipment is used for taking a set of 2D projection images that are used as input for Bayesian 3D reconstruction algorithm. Such equipment includes an intraoral X-ray unit and a digital intraoral sensor.
- 25 Benefits of this approach over conventional CT scan are
- low cost and convenient usage,
 - high resolution of the projection images,
 - possibility to take as few radiographs as is needed to capture the relevant 3D information, minimizing radiation dose to the patient,
- 30 - the possibility to choose imaging directions so that the X-rays do not pass through the whole head but only the interesting tissue, further reducing dose.

In the preferred embodiments of the invention, Bayesian inversion is used for the 3D reconstruction. Input data for the algorithm is the set of projection images and the following a priori knowledge:

- 5 (a) Dental tissue consists of few approximately homogeneous regions with well-defined boundaries.
(b) Dental tissue can only attenuate X-radiation, not intensify it.

10 The example of the detector 6 used in the first preferred embodiment of the invention is based on charge coupled device (CCD) technology and has dynamic range of 4096 gray levels. The size of the active imaging area is 34 mm * 26 mm and the resolution is 872 * 664 pixels. After exposure, each pixel contains an integer which is proportional to the number of X-ray quanta that hit the pixel's area.

15

Alternative detectors include any other digital intraoral sensor, digitized X-ray film, or any intraoral sensing device converting detected X-ray photons to a digital image.

20 In the measurement geometry the focal point of the X-ray source 2 moves horizontally on a circle in the plane 10, with center at the detector 6, see Figure 8. In Figure 8, the detector 6 corresponds to one row of CCD pixels in the CCD sensor.

25 In figure 8 is presented an example of taking seven radiographs of some teeth of a patient. The total opening angle of the projection views is 55 degrees in this example. Figure 8 represents the xy plane, and the z-coordinate axis is thought to be perpendicular to the plane of the paper.

In the preferred embodiments, mathematical modelling of the object 4 can
30 be done with a prior distribution of the form in formula (7):

$$p_{pr}(x) = \exp(-\alpha \sum_N U_N(x))$$

(7)

where the sum is taken over a collection of 3D neighbourhoods N and the value $U_N(x)$ depends only on the values of voxels belonging to the neighborhood N , and α is a positive regularization parameter used to tune the width of the prior distribution. The neighborhood N is typically a set of voxels whose center points are closer to each other than some predefined maximum distance.

10

It is to be noted that formula (7) does not define a probability distribution since it does not integrate to 1. Instead, the integral diverges. However, when used in the Bayes formula (4) with a suitable likelihood distribution, the posterior distribution is integrable. The same remark concerns the priors derived from (7), that is, formulae (9), (10) and (11).

In the preferred embodiments of the invention the three-dimensional problem can be reduced to a stack of two-dimensional problems each corresponding to a plane determined by a constant value of z . Here figure 8 represents exactly the situation in the xy plane, i.e. the plane $z=0$. Each row in the detector corresponds to one such 2D problem. This approach leads to small approximation error because the X-ray source does not move in the correct plane for nonzero z , and this error is neglected.

Next the modeling of a 2D tomographic problem is explained. Let

25

$$(8) \quad m(j) = A x(j) + e(j)$$

denote the j th 2D tomographic problem. Here the vector $m(j)$ contains the readings on j th row from each of the seven radiographs. The vector $x(j)$ is the j th slice of the 3-D representation x of the object 4 under imaging. The matrix A is the pencil beam model matrix for the 2-D tomography problem.

30

Now $x(j)$ is a 2D array of pixels. The pixels are denoted by $x(j)[k,q]$, where $k=1,2,\dots,K$ is row index and $q=1,2,\dots,Q$ is column index.

The mathematical modelling of the object 4, i.e. Incorporation of prior
5 information, is next explained for the 2D slice. Define

$$p_{pr}(x^{(j)}) = \exp(-\alpha \sum_{k=1}^K \sum_{q=1}^Q U(N(x^{(j)}[k,q])))$$

(9)

10 where the value $U(N(x(j)[k,q]))$ depends only on the values of pixels
belonging to the neighborhood N of the pixel $x(j)[k,q]$, the constant c is a
normalization constant and α is a positive regularization parameter used to
tune the width of the prior distribution. The choice of the neighborhoods
 $N(x(j)[k,q])$ is arbitrary, but a typical choice is the set of pixels whose
15 centerpoints are closer to the centerpoint of $x(j)[k,q]$ than some predefined
distance.

In the preferred embodiment, the neighborhoods are chosen to consist of
two adjacent pixels. Further, the function U is chosen to be a power of
20 absolute value of the difference between adjacent pixels. These choices lead
to formula (10):

$$25 \quad p_{pr}(x^{(j)}) = \exp \left(-\alpha \left(\sum_{k=1}^{K-1} \sum_{q=1}^Q |x^{(j)}[k,q] - x^{(j)}[k+1,q]|^s + \right. \right. \\ \left. \left. + \sum_{k=1}^K \sum_{q=1}^{Q-1} |x^{(j)}[k,q] - x^{(j)}[k,q+1]|^s \right) \right)$$

(10)

30 where s is a positive real number, and α is a regularization parameter used
to tune the width of the prior distribution.

In the equation (11) is presented non-normalized total variation (TV) distribution, when $s=1$ in equation (10). This is the case according to the preferred embodiment of the invention, because when $s=1$ the prior model becomes such that it gives high probability for objects consisting of a few areas of different attenuation with well-defined boundaries.

$$\text{prTV}(x^{(j)}) = \exp \left(-\alpha \left(\sum_{k=1}^{K-1} \sum_{q=1}^Q |x^{(j)}[k, q] - x^{(j)}[k+1, q]| + \sum_{k=1}^K \sum_{q=1}^{Q-1} |x^{(j)}[k, q] - x^{(j)}[k, q+1]| \right) \right)$$

10

(11)

X-radiation can only attenuate, not strengthen, inside tissue. This leads to positivity prior pos defined by

(12) $\text{pos}(x(j)) = 1$ if all pixels of $x(j)$ are positive, 0 otherwise.

The explanation of modeling of one 2D tomographic problem is now complete.

20 The stack of 2D problems are connected to each other by demanding that consecutive 2D slices $x(j)$ and $x(j-1)$ should not be very different. Mathematically this is expressed as follows:

$$(13) \text{pr3D}(x(j)) = \exp(-\gamma \sum \sum |x(j)[k, q] - x(j-1)[k, q]|),$$

25

where the sums are taken over $k=1, \dots, K$ and $q=1, \dots, Q$ and $\gamma > 0$ is another regularization parameter. So the prior distribution in formula (4) is the product of (11), (12) and (13):

$$30 \quad (14) \quad P_{pr}(x(j)) = \text{prTV}(x(j)) \text{pos}(x(j)) \text{pr3D}(x(j)).$$

The measurements are taken into account in the form of the likelihood distribution

$$p(m^{(j)} | x^{(j)}) = c \exp\left\{-\frac{1}{2}(m^{(j)} - Ax^{(j)})^T \Sigma^{-1}(m^{(j)} - Ax^{(j)})\right\}$$

5 (15)

where Σ is the covariance matrix of the Gaussian noise vector e . c is a normalization constant.

10 In reality, X-radiation measurement noise is Poisson distributed. Formula 15 uses a Gaussian approximation to the Poisson distribution.

All the parts are presented of the right hand side of (4). Next it is looked for the MAP estimate of $x(j)$, that is, the image $x(j)$ that gives the largest value for the posteriori distribution (4). This is equivalent to finding the image $x(j)$ that minimizes the expression

$$F(x^{(j)}) = \frac{1}{2}(m^{(j)} - Ax^{(j)})^T \Sigma^{-1}(m^{(j)} - Ax^{(j)}) + \\ - \log(\text{prTV}(x^{(j)})) - \log(\text{pr3D}(x^{(j)}))$$

(16)

20 with the additional requirement that every pixel of $x(j)$ is positive.

Minimization of (16) is difficult since F is not a differentiable function due to the absolute values present in (11) and (13) and due to the sharp cutting in (12). The absolute values in (11) and (13) are replaced by

$$25 \quad |t| \approx h_{\beta}(t) = \frac{1}{\beta} \log(\cosh(\beta t)),$$

(17)

where $\beta > 0$, enabling the use of efficient gradient-based minimization routines. The positivity constraint is taken care of by an interior search minimization method. The results are shown in figure 9 in comparison with traditional tomosynthesis technique based on backprojection.

In this description explained mathematic modelling and other image information processing are performed by software means 15 to accomplish three-dimensional information of the object 4.

5

In the second preferred embodiment the invention is utilized in dental panoramic x-ray imaging. The object 4 is typically teeth of the patient and the medical x-ray device 5 arrangement is dental panoramic x-ray device arrangement.

10

In the third preferred embodiment the invention is utilized in mammography, for example in FFDM (Full Field Digital Mammography). There the object 4 is breast of human being and the medical x-ray device 5 arrangement is mammography device arrangement.

15

In the fourth preferred embodiment the invention is utilized in surgical x-ray imaging. There the object 4 is the body part under surgery and the medical x-ray device 5 arrangement is surgical x-ray device arrangement.

20 In the first, second, third and fourth preferred embodiments of the invention the basic method steps are same as mentioned with the flow chart in figure 6. The utilizing of the invention in the second, third and fourth preferred embodiment is similar to what is described with the first preferred
25 different medical x-ray imaging applications and their differences because of different medical x-ray devices and different objects to be x-ray imaged.

30

Although the invention is described above with reference to the examples illustrated in the attached figures, it is to be understood that the invention is not limited thereto but can be varied in many ways within the inventive idea disclosed in the attached claims.

Claims

1. A method for producing three-dimensional information of an object (4) in medical X-ray imaging, **characterized in that**
- 5 - the object is modelled mathematically independently of X-ray imaging,
- the object is X-radiated from at least two different directions and the said X-radiation is detected to form projection data of the object (4),
- and said projection data and said mathematical modelling of the object are utilized in Bayesian inversion based on Bayes' formula

$$p(x | m) = \frac{p_{pr}(x) p(m | x)}{p(m)}$$

- 10 to produce three-dimensional information of the object, the prior distribution $p_{pr}(x)$ representing mathematical modelling of the object, x representing the object image vector, which comprises values of the X-ray attenuation coefficient inside the object, m representing projection data, the likelihood distribution $p(m|x)$ representing the X-radiation attenuation model between
- 15 the object image vector x and projection data m , $p(m)$ being a normalization constant and the posteriori distribution $p(x|m)$ representing the three-dimensional information of the object (4).

- 20 2. A method according to claim 1, **characterized in that** the three-dimensional information of the object (4) is one or more two-dimensional images representing X-ray attenuation coefficient along slices through the object.

- 25 3. A method according to claim 1, **characterized in that** the three-dimensional information of the object (4) is a three-dimensional voxel representation of the X-ray attenuation in the object.

- 30 4. A method according to claim 1, **characterized in that** the measurement model is $m = Ax + e$, where matrix A contains the lengths of the path of the

X-ray inside each voxel and the noise e is independent of object image vector x leading to the likelihood distribution

$$p(m | x) = p_{noise}(m - Ax)$$

5 5. A method according to claim 1, **characterized in that** the said mathematical modelling comprises that X-radiation attenuates when passing the object (4), which means that every image voxel is nonnegative.

6. A method according to claim 1, **characterized in that** mathematical
10 modelling is expressed by the formula:

$$p_{pr}(x) = \exp(-\alpha \sum_N U_N(x))$$

where the sum is taken over a collection of 3D neighbourhoods N and the
15 value $U_N(x)$ depends only on the values of voxels belonging to the neighborhood N , and α is a positive regularization parameter used to tune the width of the prior distribution.

7. A method according to claim 1, **characterized in that** the 3D
20 tomographic problem is divided into a stack of 2D tomographic problems and on every such 2D problem, the mathematical modelling is expressed by the formula:

$$p_{pr}(x) = \exp(-\alpha \sum_N U_N(x))$$

25 where the sum is taken over a collection of 2D neighbourhoods N and the value $U_N(x)$ depends only on the values of pixels belonging to the neighborhood N , and α is a positive regularization parameter used to tune the width of the prior distribution, and the 2D tomographic problems are related to each other by the formula

30

$$pr3D(x(j)) = \exp(-\gamma \sum \sum |x(j)[k,q] - x(j-1)[k,q]|),$$

where the sums are taken over all pixels ($k=1,\dots,K$, $q=1,\dots,Q$) and $\gamma > 0$ is another regularization parameter.

8. A method according to claim 7, **characterized in that** the neighborhoods
 5 consist of two adjacent pixels and U calculates a power of the absolute value of the difference, leading to the formula

$$p_{pr}(x^{(j)}) = \exp \left(-\alpha \left(\sum_{k=1}^{K-1} \sum_{q=1}^Q |x^{(j)}[k, q] - x^{(j)}[k+1, q]|^s + \right. \right. \\
 10 \quad \left. \left. + \sum_{k=1}^K \sum_{q=1}^{Q-1} |x^{(j)}[k, q] - x^{(j)}[k, q+1]|^s \right) \right)$$

where s is a positive real number.

9. A method according to claim 8, **characterized in that** $s=1$ corresponding
 15 to total variation (TV) prior describing objects (4) consisting of different regions with well-defined boundaries.

10. A method according to claim 1, **characterized in that** mathematical
 modelling is qualitative structural information of the target where the
 20 structural information is encoded in prior distributions that are concentrated around object image vectors x that correspond to the physiological structures of the object (4).

11. A method according to claim 1, **characterized in that** mathematical
 25 modelling consists of a list or probability distribution of possible attenuation coefficient values in the object (4).

12. A method according to claim 1, **characterized in that** the X-ray
 imaging geometry, such as X-ray source position, has unknown error
 30 modelled in the distribution $p(m|x)$.

13. A method according to claim 1, **characterized in that** the X-radiation measurement noise is Poisson distributed.
14. A method according to claim 1, **characterized in that** the medical X-ray imaging is dental radiography.
15. A method according to claim 1, **characterized in that** the medical X-ray imaging is surgical C-arm imaging.
16. A method according to claim 1, **characterized in that** the medical X-ray imaging is mammography.
17. A method according to claim 1, **characterized in that** three-dimensional information of the object (4) is produced on the basis of the maximum a posteriori estimator (MAP) which is calculated by the equation:

$$p(x_{\text{MAP}} | m) = \max p(x | m),$$

m representing projection data and x representing the object image vector and where the maximum on the right hand side of the equation is taken over all x.

18. A method according to claim 1, **characterized in that** three-dimensional information of the object (4) is produced on the basis of the conditional mean estimator (CM), which is calculated by the equation:

$$x_{\text{CM}} = \int x p(x | m) dx$$

where m represents projection data and x represents the object image vector.

19. A medical X-ray device (5) arrangement for producing three-dimensional information of an object (4) in a medical X-ray imaging, **characterized in that** the medical X-ray device (5) arrangement comprises:

- 5 - means (15) for modelling the object (4) mathematically independently of X-ray imaging
- an X-ray source (2) for X-radiating the object from at least two different directions
- a detector (6) for detecting the X-radiation to form projection data of the object (4)
- 10 - and means (15) for utilizing said projection data and said mathematical modelling of the object in Bayesian Inversion based on Bayes' formula

$$p(x|m) = \frac{p_{pr}(x)p(m|x)}{p(m)}$$

- 15 to produce three-dimensional information of the object, the prior distribution $p_{pr}(x)$ representing mathematical modelling of the object, x representing the object image vector, which comprises values of the X-ray attenuation coefficient inside the object, m representing projection data, the likelihood distribution $p(m|x)$ representing the X-radiation attenuation model between
- 20 the object image vector x and projection data m , $p(m)$ being a normalization constant and the posteriori distribution $p(x|m)$ representing the three-dimensional information of the object (4).

20. A medical x-ray device (5) arrangement according to claim 19,
- 25 **characterized in that** the three-dimensional information of the object (4) is one or more two-dimensional images representing X-ray attenuation coefficient along slices through the object.

21. A medical x-ray device (5) arrangement according to claim 19,
- 30 **characterized in that** the three-dimensional information of the object (4) is

a three-dimensional voxel representation of the X-ray attenuation in the object.

22. A medical X-ray device (5) arrangement according to claim 19,
 5 **characterized in that** the medical X-ray device arrangement comprises means (15) for modelling the measurement as
 $m = Ax + e$,
 where matrix A contains the lengths of the path of the X-ray inside each voxel and the noise e is independent of object image vector x leading to the
 10 likelihood distribution

$$p(m | x) = p_{noise}(m - Ax).$$

23. A medical X-ray device (5) arrangement according to claim 19
 15 **characterized in that** the medical X-ray device arrangement comprises means (15) for modelling the object (4) mathematically so that X-radiation attenuates when passing the object (4), which means that every image voxel is nonnegative.

- 20 24. A medical X-ray device (5) arrangement according to claim 19, **characterized in that** the medical X-ray device arrangement comprises means (15) for modelling the object (4) mathematically by the formula:

$$p_{pr}(x) = \exp(-\alpha \sum_N U_N(x))$$

25

where the sum is taken over a collection of 3D neighbourhoods N and the value $U_N(x)$ depends only on the values of voxels belonging to the neighborhood N, and α is a positive regularization parameter used to tune the width of the prior distribution.

- 30 25. A medical x-ray device (5) arrangement according to claim 19, **characterized in that** the 3D tomographic problem is divided into a stack

of 2D tomographic problems and on every such 2D problem, and the medical X-ray device arrangement comprises means (15) for modelling the object (4) mathematically by the formula:

$$p_{pr}(x) = \exp(-\alpha \sum_N U_N(x))$$

where the sum is taken over a collection of 2D neighbourhoods N and the value $U_N(x)$ depends only on the values of pixels belonging to the neighborhood N, and α is a positive regularization parameter used to tune the width of the prior distribution, and the 2D tomographic problems are related to each other by the formula

$$pr3D(x(j)) = \exp(-\gamma \sum \sum |x(j)[k,q] - x(j-1)[k,q]|),$$

where the sums are taken over all pixels ($k=1,...,K$, $q=1,...,Q$) and $\gamma > 0$ is another regularization parameter.

26. A medical X-ray device (5) arrangement according to claim 25, **characterized in that** the neighborhood systems consist of two

neighboring pixels x_j , x_k or voxels x_j , x_k and $U_N(x)$ calculates a power of the

$$p_{pr}(x^{(j)}) = \exp \left(-\alpha \left(\sum_{k=1}^{K-1} \sum_{q=1}^Q |x^{(j)}[k,q] - x^{(j)}[k+1,q]|^s + \sum_{k=1}^K \sum_{q=1}^{Q-1} |x^{(j)}[k,q] - x^{(j)}[k,q+1]|^s \right) \right)$$

25

absolute value of the difference, leading to the formula where s is a positive real number and α is a regularization parameter used to tune the width of the prior distribution.

27. A medical X-ray device (5) arrangement according to claim 26, **characterized in that** the medical X-ray device arrangement comprises means (15) for modelling the object (4) mathematically by setting $s=1$

corresponding to total variation (TV) prior describing objects consisting of different regions with well-defined boundaries.

28. A medical X-ray device (5) arrangement according to claim 19,
5 **characterized in that** the medical X-ray device arrangement comprises means (15) for modelling the object (4) mathematically by assuming that mathematical modelling is qualitative structural information of the target where the structural information is encoded in prior distributions that are concentrated around image vectors x that correspond to the physiological
10 structures of the target.

29. A medical X-ray device (5) arrangement according to claim 19,
characterized in that the medical X-ray device arrangement comprises means (15) for modelling the object (4) mathematically by assuming that
15 mathematical modelling consists of a list of possible attenuation coefficient values in the object.

30. A medical X-ray device (5) arrangement according to claim 19,
characterized in that the medical X-ray device arrangement comprises
20 means (15) for modelling the object (4) mathematically by assuming that the X-ray imaging geometry, such as X-ray source position, has unknown error modelled in the distribution $p(m|x)$.

31. A medical X-ray device (5) arrangement according to claim 19,
25 **characterized in that** the medical X-ray device arrangement comprises means (15) for modelling the object (4) mathematically by assuming that X-radiation measurement noise is Poisson distributed.

32. A medical X-ray device (5) arrangement according to claim 19,
30 **characterized in that** the medical X-ray imaging is dental radiography.

33. A medical X-ray device (5) arrangement according to claim 19,
characterized in that the medical X-ray imaging is surgical C-arm imaging.

34. A medical X-ray device (5) arrangement according to claim 19,
 5 **characterized in that** the medical X-ray imaging is mammography.

35. A medical X-ray device (5) arrangement according to claim 19,
characterized in that the medical X-ray device arrangement comprises
 means (15) for producing three-dimensional information of the object (4) on
 10 the basis of the maximum a posteriori estimator (MAP), which is calculated
 by the equation:

$$p(x_{\text{MAP}} | m) = \max p(x | m),$$

15 m representing projection data and x representing the object image vector
 and where the maximum on the right hand side of the equation is taken over
 all x.

36. A medical X-ray device (5) arrangement according to claim 19,
 20 **characterized in that** the medical X-ray device arrangement comprises
 means (15) for producing three-dimensional information of the object (4) on
 the basis of the conditional mean estimator (CM), which is calculated by the
 equation

25
$$x_{\text{CM}} = \int x p(x | m) dx$$

where m represents projection data and x represents the object image
 vector.

1/9

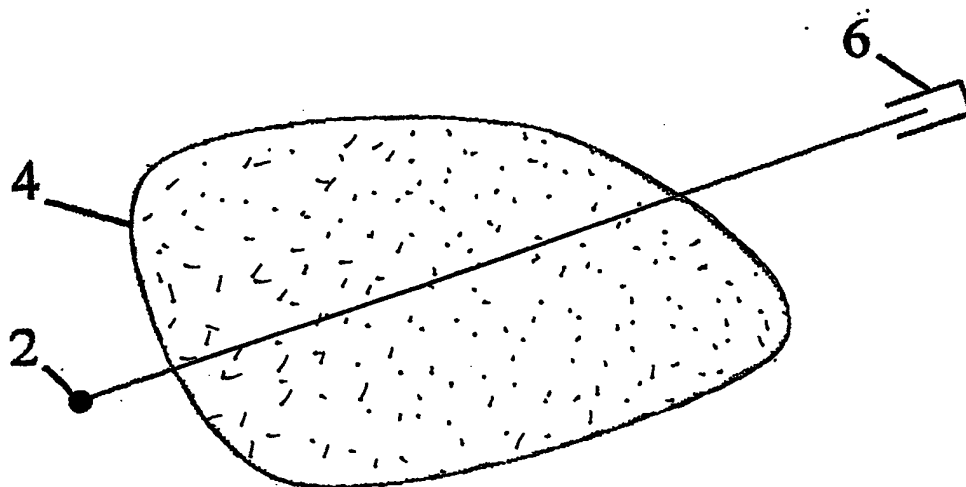


Fig. 1

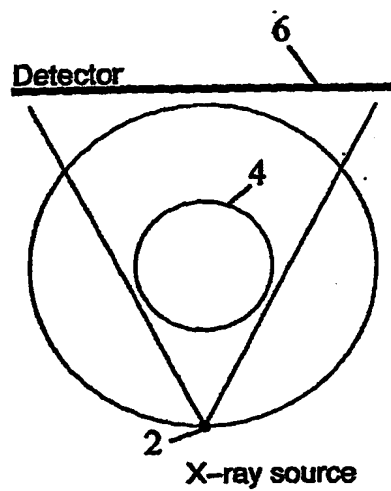


Fig. 2A

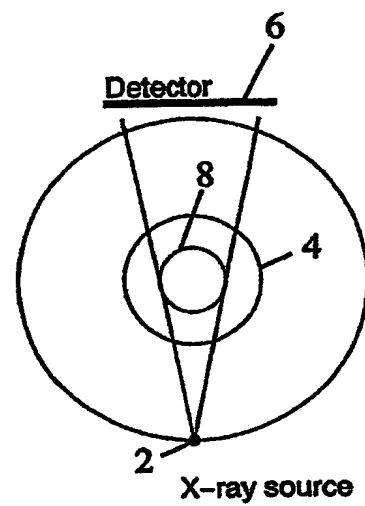


Fig. 2B

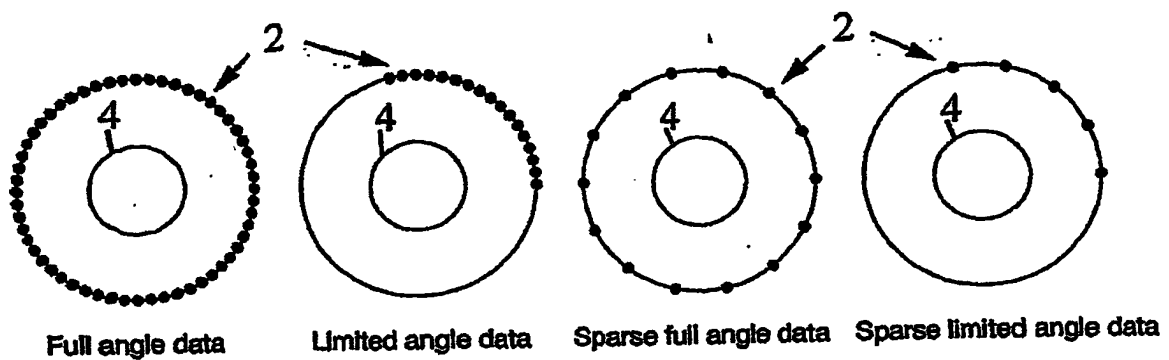


Fig.3A

Fig.3B

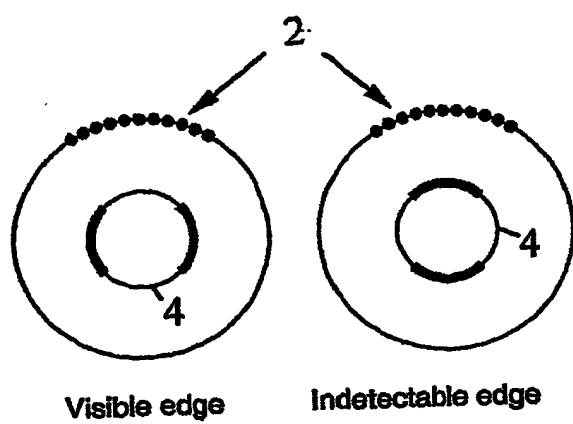


Fig. 4a

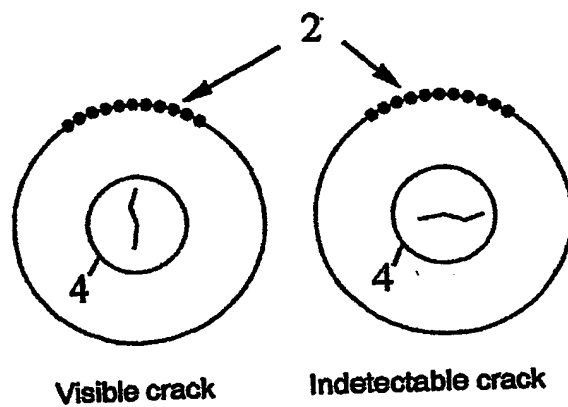


Fig. 4B

5/9

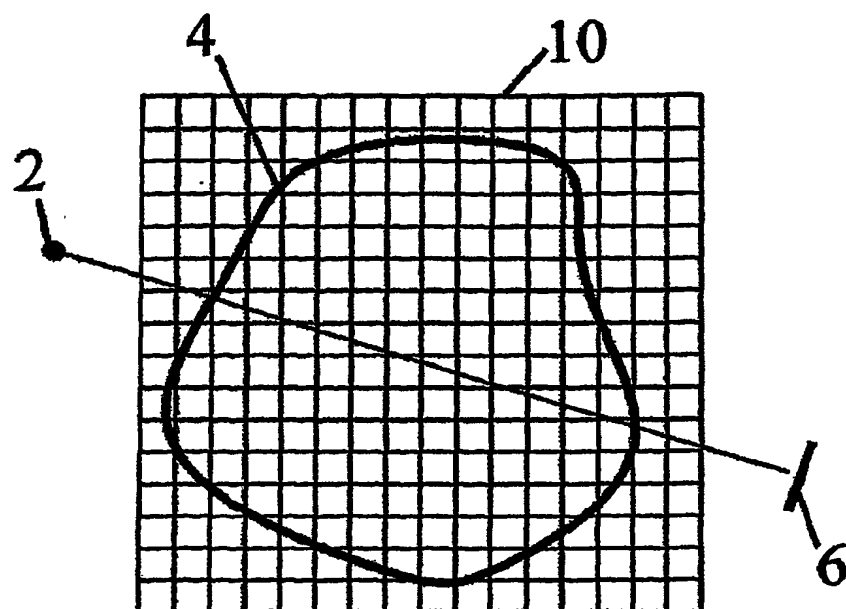
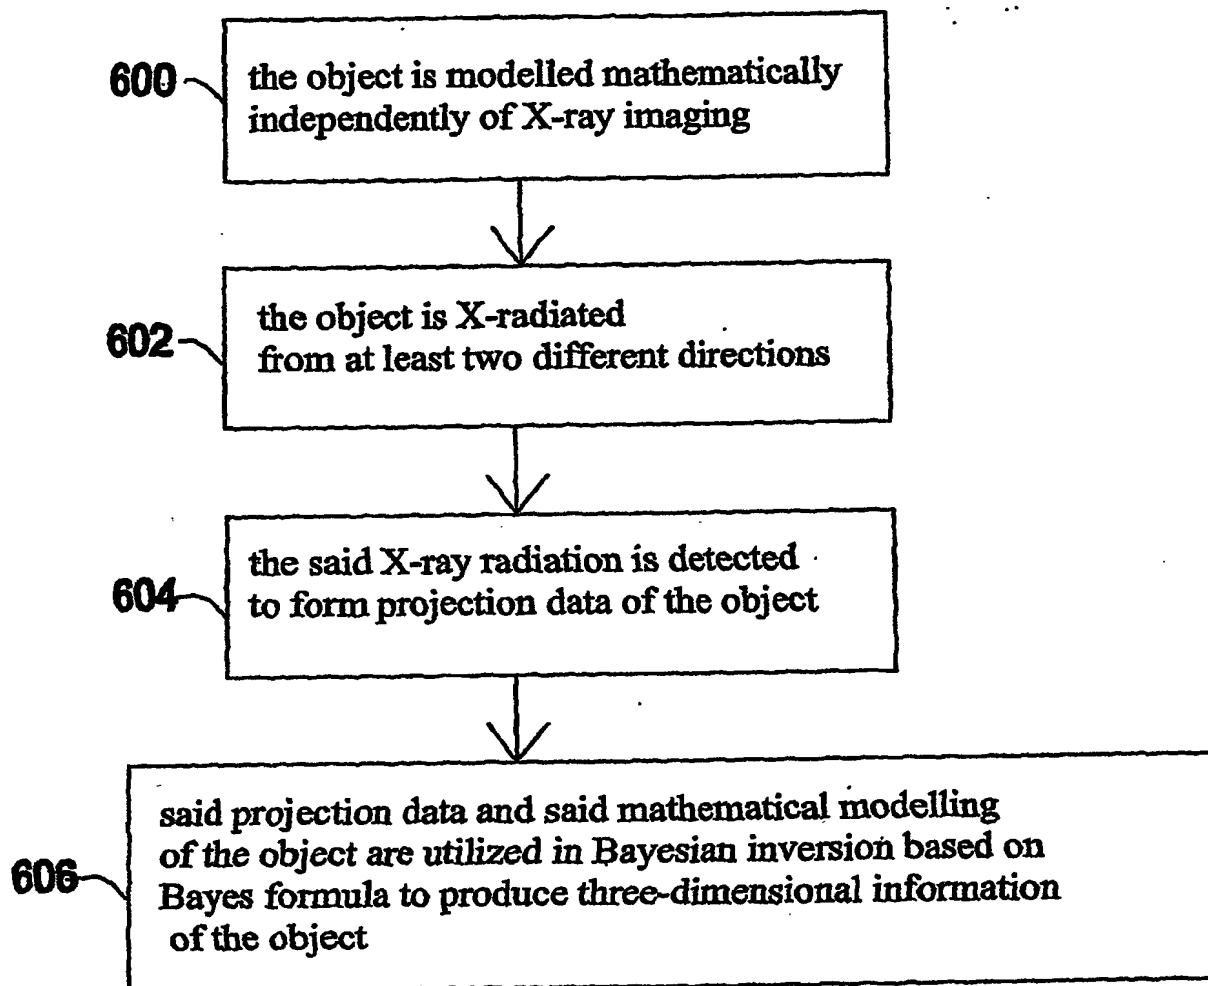


Fig.5

6/9

*Fig.6*

7/9

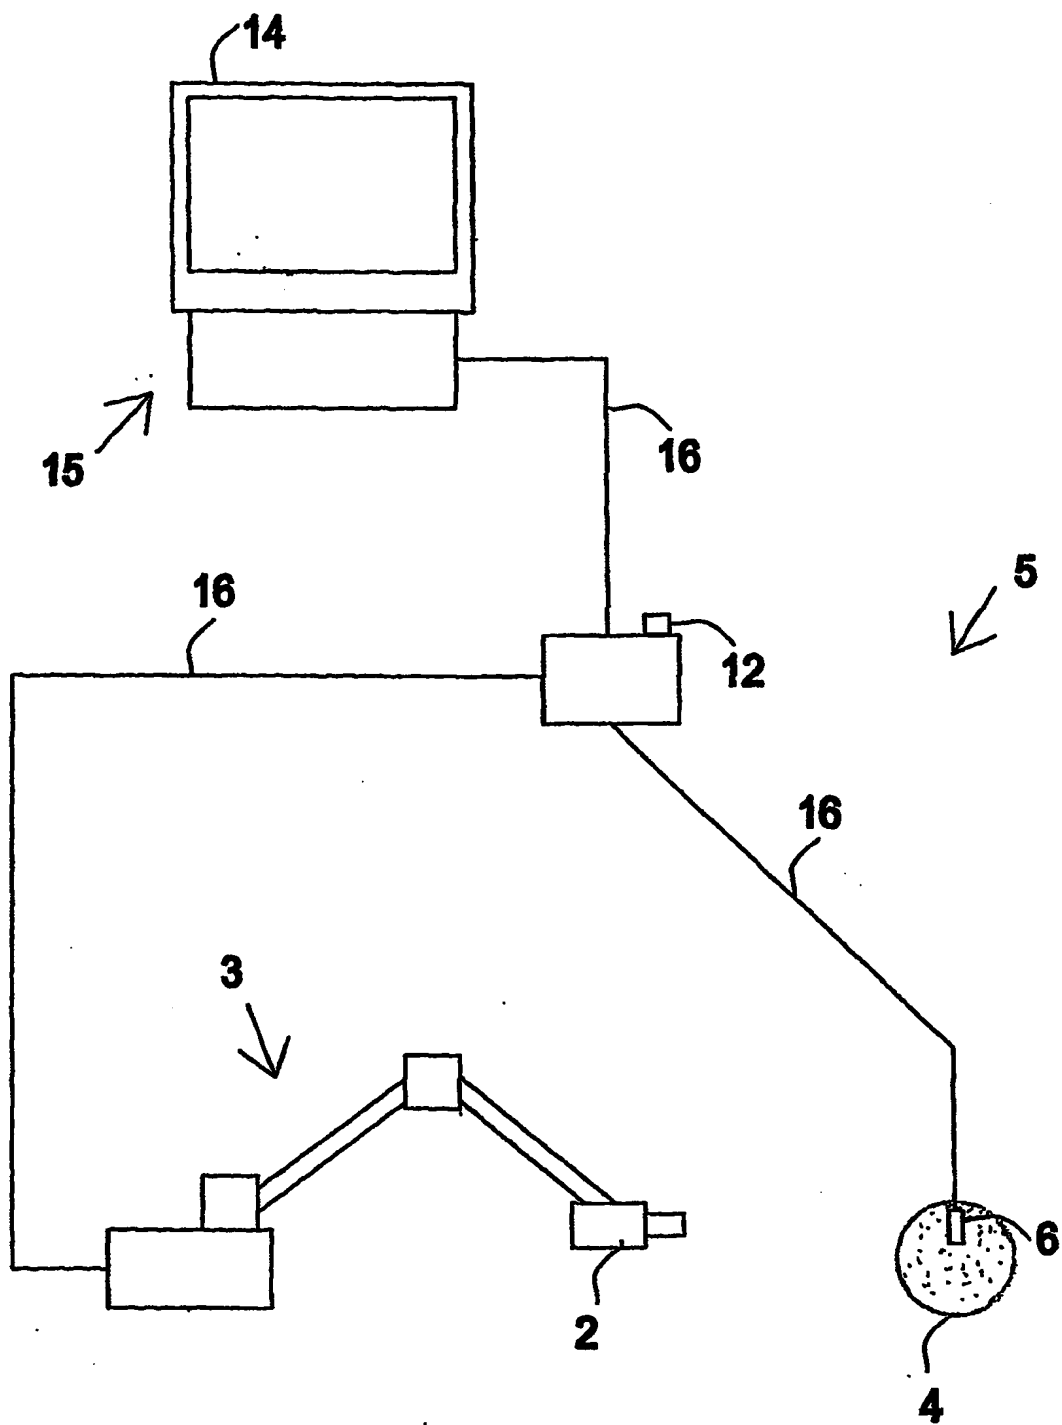


Fig.7


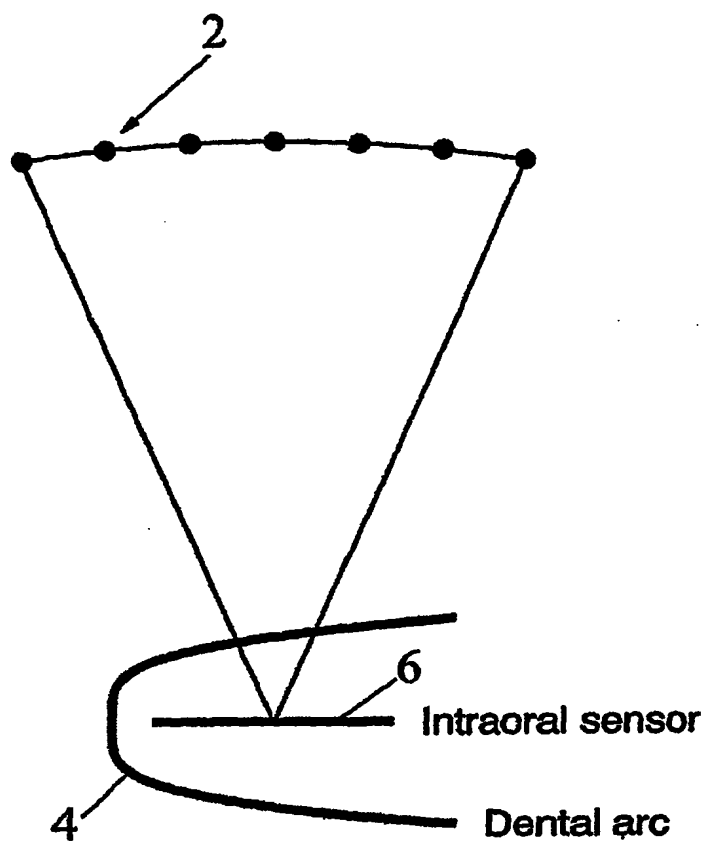


Fig.8

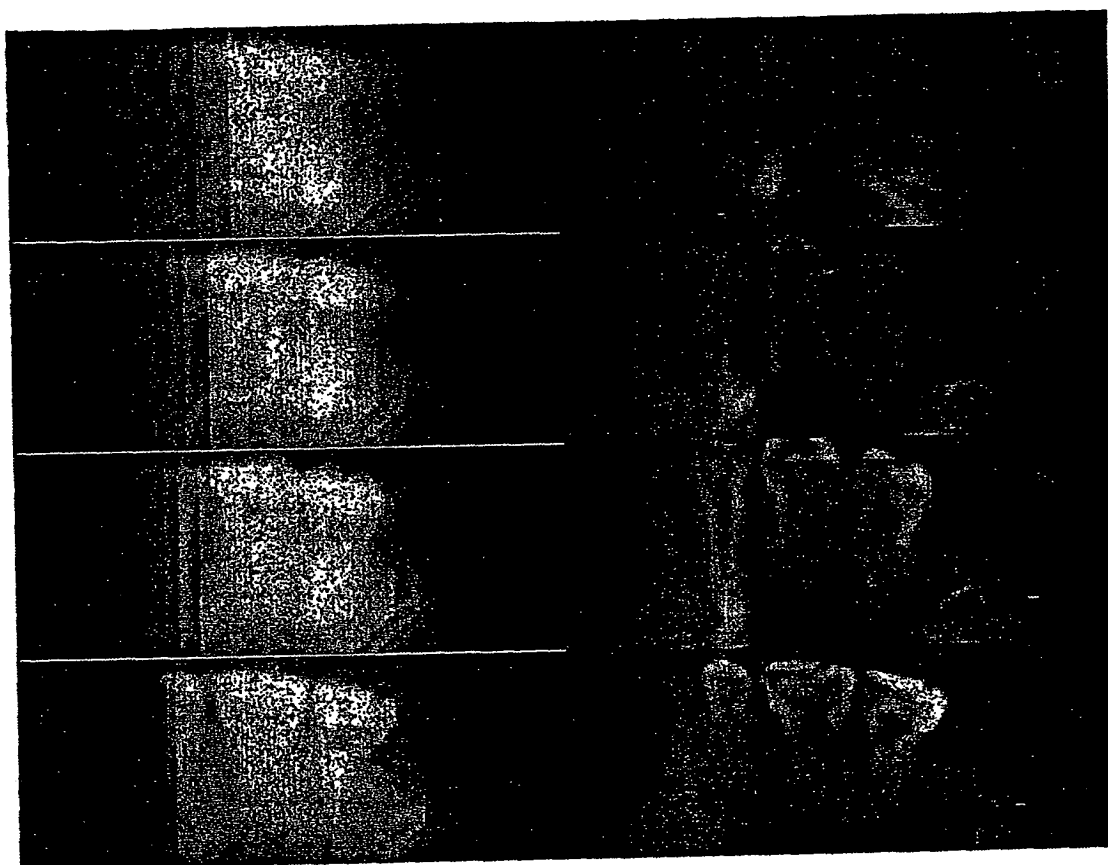

Traditional tomosynthesis

Invention

FIGURE 9

INTERNATIONAL SEARCH REPORT

International application No.

PCT/FI 03/00625

A. CLASSIFICATION OF SUBJECT MATTER

IPC7: A61B 6/03, G06T 17/00

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

IPC7: A61B, G06T, G06F

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

SE,DK,FI,NO classes as above

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)

EPO-INTERNAL, WPI, INSPEC, MEDLINE

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
A	"HYBRID INTERPOLATIONS TO ENHANCE 3 D MEDICAL IMAGE RECONSTRUCTION." in: CHIN. J. MED. BIOL. ENG. (TAIWAN), CHINESE JOURNAL OF MEDICAL AND BIOLOGICAL ENGINEERING, March 2000, Biomed. Eng. Soc. Republic of China, Taiwan Don-Lin Yang et al. ISSN 1019-0465 retrieved on 2003-11-17 --	1-38
A	DATABASE INSPEC/IEE "TOTAL VARIATION NORM FOR THREE-DIMENSIONAL ITERATIVE RECONSTRUCTION IN LIMITED VIEW ANGEL TOMOGRAPHY." Phys. Med. Biol. (UK), Physics in Medicine and Biology, March 2001, IOP Publishing, UK. ISSN 0031-9155 vol 46, nr. 3 --	1-38

☒ Further documents are listed in the continuation of Box C.

☒ See patent family annex.

* Special categories of cited documents:

- "A" document defining the general state of the art which is not considered to be of particular relevance
- "E" earlier application or patent but published on or after the international filing date
- "L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)
- "O" document referring to an oral disclosure, use, exhibition or other means
- "P" document published prior to the international filing date but later than the priority date claimed

- "T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention
- "X" document of particular relevance: the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone
- "Y" document of particular relevance: the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art
- "&" document member of the same patent family

Date of the actual completion of the international search

18 November 2003

Date of mailing of the international search report

21-11-2003

Name and mailing address of the ISA/
Swedish Patent Office
Box 5055, S-102 42 STOCKHOLM
Facsimile No. +46 8 666 02 86

Authorized officer

Patrik Widerdal /itw
Telephone No. +46 8 782 25 00

INTERNATIONAL SEARCH REPORT

International application No.

PCT/FI 03/00625

C (Continuation). DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
A	<p>"A scale invariant bayesian method to solve linear inverse problems." Mohammad-Djafari et al. Presented at the 13th International Workshop on Maximum Entropy and Bayesian Methods (MaxEnt93) USA 1995 US 2002/0015006 A1 Abstract</p> <p>--</p>	1-38
A	<p>WO 0077719 A1 (THE REGENTS OF THE UNIVERSITY OF CALIFORNIA), 21 December 2000 (21.12.00), figure 1, abstract</p> <p>--</p>	1-38
A	<p>DATABASE INSPEC/IEE "THREE DIMENSIONAL VOLUMETRIC MODELING OF THE INTERNAL BRAIN STRUCTURE USING MAGNETIC RESONANCE.." 2001 Conference Proceedings of the 23rd Annual International Conference of the IEEE Engineering in Medicine and Biology Society, Istanbul, Turkey, 25-28 Oct. International Conference of the IEEE Engineering in Medicine and Biology Society, Istanbul, TURKEY, 25-28 Oct. 2001. Sallam A A et al. Abstract</p> <p>--</p>	1-38
A	<p>DATABASE INSPEC/IEE "RECONSTRUCTION OF 3-D LEFT VENTRICULAR MOTION FROM PLANAR TAGGED CARDIAC MR IMAGES: AN ESTIMATION THEORETIC APPROACH." IEEE Trans. Med. Imaging (USA, IEEE Transactions on Medical imaging, Dec. 1995, IEEE, USA Denney TS et al ISSN 0278-0062 Abstract</p> <p>-- -----</p>	1-38

INTERNATIONAL SEARCH REPORT

Information on patent family members

06/09/03

International application No.

PCT/FI 03/00625

Patent document cited in search report			Publication date	Patent family member(s)		Publication date
WO	0077719	A1	21/12/00	AU	5315200 A	02/01/01
				US	6353688 B	05/03/02
				US	6490374 B	03/12/02
				US	2002044698 A	18/04/02
